

JITEKIE-ISSN: 2338-3062
P-ISSN: 2338-3070

Jurnal Ilmiah Teknik Elektro Komputer dan Informatika

<http://journal.uad.ac.id/index.php/JITEKI>[HOME](#) [ABOUT](#) [LOGIN](#) [REGISTER](#) [SEARCH](#) [CURRENT](#) [ARCHIVES](#) [ANNOUNCEMENTS](#) [JOURNAL HISTORY](#) [VIDEO ABSTRACT](#)[Home > Vol 8, No 2 \(2022\)](#)

Jurnal Ilmiah Teknik Elektro Komputer dan Informatika

Journal title	Jurnal Ilmiah Teknik Elektro Komputer dan Informatika
Initials	JITEKI
Frequency	4 issues per year (March, June, September and December)
DOI	10.26555/jiteki
Print ISSN	2338-3070
Online ISSN	2338-3062
Business Model	Open Access & Author-Pays
License	CC-BY-SA
Editor-in-chief	Deris Stiawan
Managing Editor	Alfian Ma'arif Son Ali Akbar
Publisher	Universitas Ahmad Dahlan
Citation Analysis	SINTA GOOGLE SCHOLAR SCOPUS DIMENSIONS

Jurnal Ilmiah Teknik Elektro Komputer dan Informatika (JITEKI Journal) is a peer-reviewed open-access journal that is published four times a year (March, June, September, and December). The scientific journal is published by Universitas Ahmad Dahlan (UAD). The JITEKI aims to provide a national and international forum for academics, researchers, and professionals to share their ideas on all topics related to Electrical, Computer, and Informatics Engineering. It publishes its issues in an online (e-ISSN [2338-3062](#)) and a printed (p-ISSN [2338-3070](#)) version.

Sinta Impact = 1.35**Dimensions Impact = 0.69****Days to First Decision = 36****Days to Publication = 57****Acceptance Rate = 50%**

After being founded in 2015, the journal has been indexed in some databases such as [GOOGLE Scholar](#), [GARUDA](#) (Digital National Library), [Bielefeld Search Engine \(BASE\)](#), [Dimensions](#), [WorldCat](#), [Crossref Search](#), [One Search](#) (National Library of Indonesia), [Moraref](#) (Religious Ministry of Indonesia) and etc.

In 2016, JITEKI has been accredited by the National Journal Accreditation (ARJUNA) managed by the Ministry of Research, Technology, and Higher Education (RISTEKDIKT), Republic Indonesia with Fourth Grade (**SINTA 4**) according to [decree No. 21/E/KPT/2018](#).

In 2020, JITEKI has been reaccredited and reached Second Grade (**SINTA 2**) according to [decree No. 200/M/KPT/2020](#) by the National Journal Accreditation (ARJUNA) managed by the Ministry of Research, and Technology / National Research and Innovation Agency (RISTEK/BRIN), Republic Indonesia.

The JITEKI welcomes high-quality manuscripts resulting from a research project. The manuscript must be an original research or review manuscript, written in English, and not be simultaneously submitted to another journal or conference. All submitted manuscripts will be initially reviewed by editors and are then evaluated by a minimum of two reviewers through the single-blind review process. This is to ensure the quality of the published manuscripts in the journal.

Before Submission, The author has to make sure that the manuscript has been prepared using [the JITEKI template](#) following the [author guidelines](#). The manuscript should also have been carefully proofread. Any manuscript which does not meet the author guidelines is written in a different format, has poor soundness of English, or has a high [plagiarism percentage](#) (more than 25%), will be immediately rejected. The only manuscript which meets the [JITEKI format](#) will be processed further.

Online Submissions

1. Already have a Username/Password? [GO TO LOGIN](#)
2. Need a Username/Password? [GO TO REGISTRATION](#)

Registration and login are required to submit items online and to check the status of current submissions. Please see the tutorial for submission here <https://youtu.be/yaP0JPoK6mQ>.



SINTA CERTIFICATE



Focus and Scope

Editorial Boards

Reviewers

Author Guidelines

Online Submissions

Publication Ethics

Open Access Policy

Copyright Notice

Visitor Statistics

Author Fee

Contact Us

ABSTRACTING AND INDEXING

- » [SINTA](#)
- » [Google Scholar](#)
- » [GARUDA](#)
- » [Dimensions](#)
- » [Microsoft Academic Search](#)
- » [One Search](#)
- » [PKP-Indexed](#)
- » [Crossref](#)
- » [Moraref](#)
- » [Publons](#)
- » [Scilit](#)
- » [WorldCat](#)
- » [Index Copernicus](#)

USER

Username

Password

☐ Remember me

JOURNAL TEMPLATE



NOTIFICATIONS

- » [View](#)
- » [Subscribe](#)

JOURNAL CONTENT

Search

JITEKI

E-ISSN: 2338-3062
P-ISSN: 2338-3070

Jurnal Ilmiah Teknik Elektro Komputer dan Informatika
<http://journal.uad.ac.id/index.php/JITEKI>



[HOME](#) [ABOUT](#) [LOGIN](#) [REGISTER](#) [SEARCH](#) [CURRENT](#) [ARCHIVES](#) [ANNOUNCEMENTS](#) [JOURNAL HISTORY](#) [VIDEO ABSTRACT](#)

[Home](#) > [About the Journal](#) > **Editorial Team**

Editorial Team

Editor-in-Chief

Dr. Deris Stiawan, (SCOPUS ID: 36449642900), Universitas Sriwijaya, Indonesia

Managing Editor

Assist. Prof. Alfian Ma'arif, Universitas Ahmad Dahlan, Indonesia

Son Ali Akbar, (SCOPUS ID: 57203215193), Universitas Ahmad Dahlan, Indonesia

Associate Editors

Prof. Dr. Marco Antonio Márquez Vera, (SCOPUS ID: 55794764800), Polytechnic University of Pachuca, Mexico

Prof. Dr. Kamarul Hawari Bin Ghazali, (SCOPUS ID: 24070207000), Universiti Malaysia Pahang, Malaysia

Prof. Dr. Ismail Rakip Karas, (SCOPUS ID: 37074847400), Karabuk University (KBÜ), Turkey

Prof. Dr. Goutam Chakraborty, (SCOPUS ID: 35565864200), Iwate Prefectural University, Japan

Prof. Dr. Seifedine Kadry, (SCOPUS ID: 55906598300), Noroff University College, Norway

Assist. Prof. Dr. Khan Muhammad, (SCOPUS ID: 56651946700), Sejong University, Korea, Republic of

Assist. Prof. Dr. Szczepan Paszkiel, (SCOPUS ID: 23988042700), Opole University of Technology, Poland

Dr. Reza Alayi, Department of Mechanics, Germe Branch, Islamic Azad University, Germe, Iran, Islamic Republic of

Editorial Board Member 1

Prof. Dr. Jufriadif Na'am, (SCOPUS ID: 57189371499), Universitas Putra Indonesia YPTK Padang, Indonesia

Dr. Zhixiong Li, University of Wollongong, Australia

Dr. Mohd Norzali, (SCOPUS ID: 57195534081), Universiti Tun Hussein Onn Malaysia (UTHM), Malaysia

Dr. R. Bhoopathi, (SCOPUS ID: 56505578700), Sri Sairam Engineering College, India

Dr. Hairul Nizam Mohd Shah, (SCOPUS ID: 57189726649), Universiti Teknikal Malaysia Melaka (UTeM), Malaysia

Dr. Evizal Abdul Kadir, (SCOPUS ID: 50561254400), Universitas Islam Riau, Indonesia

Dr. Ramzi Adriman, (SCOPUS ID: 55880088400), Universitas Syiah Kuala, Indonesia

Dr. Tresna Dewi, (SCOPUS ID: 56106827800), Politeknik Negeri Sriwijaya, Indonesia

Dr. Zulfatman Zulfatman, (SCOPUS ID: 57209705112), Universitas Muhammadiyah Malang, Indonesia

Dr. Arief Marwanto, (SCOPUS ID: 36023868500), Universitas Islam Sultan Agung Semarang, Indonesia

Dr. Srirustha Sukaridhoto, (SCOPUS ID: 35100882700), Politeknik Elektronika Negeri Surabaya (PENS), Indonesia

Dr. Iswanto - Iswanto, (SCOPUS ID: 56596730700), Universitas Muhammadiyah Yogyakarta, Indonesia

Mr. Omar Muhammed Neda, (SCOPUS ID: 57208327668), Sunni Diwan Endowment, Iraq

Asst. Prof. Haider Alrikabi, Wasit University (SCOPUS ID: 57211627309), Iraq

Rania Majdoubi, (SCOPUS ID: 57219051894), Mohammed V University in Rabat, Morocco

Saddam Hussain, (SCOPUS ID: 57217510430), Hazara University Mansehra, Pakistan

Jonattan Niño Parada, Universidad de Los Llanos, Colombia

Editorial Board Member 2

Mrs. R S M Lakshmi Patibandla, Vignan's Foundation for Science Technology and Research, India

Copy Editor

Phisca Aditya Rosyady, Universitas Ahmad Dahlan

Jurnal Ilmiah Teknik Elektro Komputer dan Informatika

ISSN 2338-3070 (print) | 2338-3062 (online)

Organized by [Electrical Engineering Department](#) - Universitas Ahmad Dahlan

Published by [Universitas Ahmad Dahlan](#)

Website: <http://journal.uad.ac.id/index.php/jiteki>

Email 1: jiteki@ee.uad.ac.id

Email 2: alfianmaarif@ee.uad.ac.id

Office Address: Kantor Program Studi Teknik Elektro, Lantai 6 Sayap Barat, Kampus 4 UAD, Jl. Ringroad Selatan, Tamanan, Kec. Banguntapan, Bantul, Daerah Istimewa Yogyakarta 55191, Indonesia

SINTA CERTIFICATE



Focus and Scope

Editorial Boards

Reviewers

Author Guidelines

Online Submissions

Publication Ethics

Open Access Policy

Copyright Notice

Visitor Statistics

Author Fee

Contact Us

ABSTRACTING AND INDEXING

- » SINTA
- » Google Scholar
- » GARUDA
- » Dimensions
- » Microsoft Academic Search
- » One Search
- » PKP-Indexed
- » Crossref
- » Moraref
- » Publons
- » Scilit
- » WorldCat
- » Index Copernicus

USER

Username

Password

☐ Remember me

JOURNAL TEMPLATE



NOTIFICATIONS

- » [View](#)
- » [Subscribe](#)

JOURNAL CONTENT

Search

Search Scope

All

Search

Browse

» By Issue

» By Author

» By Title

» Other Journals

KEYWORDS

COVID-19 Control Distributed Generation GLCM GloVe Image Processing Internet of Things IoT Machine Learning Monitoring Naive Bayes Obstacle Avoidance PID PLC Particle Swarm Optimization Prediction Security Sentiment Analysis Temperature Text Classification optimization

VISITOR

View JITEKI stat

0000270928

VISITOR COUNTRY

Visitors

	26,336		274
	2,641		245
	914		195
	428		185
	387		185
	370		144
	317		135
	305		130
	285		119
	279		119

FLAG counter

JITEKI

E-ISSN: 2338-3062

P-ISSN: 2338-3070

Jurnal Ilmiah Teknik Elektro Komputer dan Informatika

http://journal.uad.ac.id/index.php/JITEKI

 **sinta** Science and Technology Index

 **S2**

 **Google** scholar

 **GARUDA** GARRA RUJUKAN DIGITAL

HOME

ABOUT

LOGIN

REGISTER

SEARCH

CURRENT

ARCHIVES

ANNOUNCEMENTS

JOURNAL HISTORY

VIDEO ABSTRACT

Home > Archives > Vol 8, No 2 (2022)

Vol 8, No 2 (2022)

June

The issue is **in progress**.

The author's countries come from INDONESIA, POLAND, BANGLADESH, PHILIPHINES, UZBEKISTAN, TAIWAN, JAPAN, IRAQ.

Table of Contents

Articles

K-Means Segmentation Based-on Lab Color Space for Embryo Detection in Incubated Egg	PDF
<i>Shoffan Saifullah, Rafal Drezewski, Alin Khaliduzzaman, Lean Karlo Tolentino, Rabbimov Ilyos</i>	175-185
Analysis of Combination Algorithms for Denoising and Contrast Enhancement Images	PDF
<i>Irpan Adiputra Pardosi, Hernawati Gohzali</i>	186-198
Blockchain Technology	PDF
<i>Purwono Purwono, Alfian Ma'arif, Wahyu Rahmانيar, Qazi Mazhar ul Haq, Dimas Herjuno, Muchammad Naseer</i>	199-205
Modeling and Analysis of Percentage Depth Dose (PDD) and Dose Profile of X-Ray Beam Produced by Linac Device with Voltage Variation	PDF
<i>Bilalodin Bilalodin, Farzand Abdullatif</i>	206-214
Comparison of IDW and Kriging Interpolation Methods Using Geoelectric Data to Determine the Depth of the Aquifer in Semarang, Indonesia	PDF
<i>Brilliananta Radix Dewana, Sri Yulianto Joko Prasetyo, Kristoko Dwi Hartomo</i>	215-225
Valuation of 5G mmWave Fixed Wireless Access in Residence Area: Analysis of Real Option for Wireless Broadband Service in Kota Wisata Cibubur Using Decision Tree and Black Scholes Model	PDF
<i>May Hendra Panjaitan, Catur Apriono</i>	226-234
Embedded Instrumentation System Using Acquisition Mechanism for BLDC-Powered Electric Vehicle	PDF
<i>Agus Ulinuha, Ibnu Shokhibul Khak</i>	235-248
Simulation and Optimization of Rectangular Microstrip Patch Antenna for Mobile 5G Communications	PDF
<i>Hamzah M. Marhoon, Noorulden Basil, Ahmed R. Ibrahim, Hussein A. Abdualnabi</i>	249-255
Application-based Simulation on the Digital Trunking Radio Communication System to Predict the Area Coverage	PDF
<i>Arief Goeritno, Nesia Andriana, Indriya Indriya, Ika Setyawibawa, Dwi Suhartono</i>	256-268
Production Stock Monitoring System at PT Yamaha Indonesia Using the Scrum Method	PDF
<i>Rizkina Maulida Safira, Chanifah Indah Ratnasari</i>	269-281
Towards Service Level Agreement Quantification on Service-Based Computing	PDF
<i>Irving Vitra Paputungan, Akmal Kurniadi Denna, Devi Rachmawati</i>	282-289
Tuberculosis Detection in X-Ray Image Using Deep Learning Approach with VGG-16 Architecture	PDF
<i>Suci Aulia, Sugondo Hadiyoso</i>	290-297
A Hybrid DenseNet201-SVM for Robust Weed and Potato Plant Classification	PDF
<i>Muhammad Dzulfikar Fauzi, Faisal Dharma Adhinata, Nur Ghaniyiyanto Ramadhan, Nia Annisa Ferani Tanjung</i>	298-306
UDP Pervasive Protocol Design and Implementation on Multi Devices using MyRIO	
<i>Mochammad Hannats Hanafi Ichsan, Rizal Maulana, Octavian Metta Wisnu Wardhana</i>	

SINTA CERTIFICATE



Focus and Scope

Editorial Boards

Reviewers

Author Guidelines

Online Submissions

Publication Ethics

Open Access Policy

Copyright Notice

Visitor Statistics

Author Fee

Contact Us

ABSTRACTING AND INDEXING

» SINTA

» Google Scholar

» GARUDA

» Dimensions

» Microsoft Academic Search

» One Search

» PKP-Indexed

» Crossref

» Moraref

» Publons

» Scilit

» WorldCat

» Index Copernicus

USER

Username

Password

☐ Remember me

Login

JOURNAL TEMPLATE



NOTIFICATIONS

» View

» Subscribe

JOURNAL CONTENT

Search

Anti-Forensics With Steganographic File Embedding in Digital Image Using Genetic Algorithm

Amadeus Pondera Purnacandra, Subektiningsih Subektiningsih

Lung Sounds Classification Based on Time Domain Features

Achmad Rizal, Istiqomah Istiqomah

Jurnal Ilmiah Teknik Elektro Komputer dan Informatika

ISSN 2338-3070 (print) | 2338-3062 (online)
Organized by Electrical Engineering Department - Universitas Ahmad Dahlan
Published by Universitas Ahmad Dahlan
Website: <http://journal.uad.ac.id/index.php/jiteki>
Email 1: jiteki@ee.uad.ac.id
Email 2: alfianmaarif@ee.uad.ac.id
Office Address: Kantor Program Studi Teknik Elektro, Lantai 6 Sayap Barat, Kampus 4 UAD, Jl. Ringroad Selatan, Tamanan, Kec. Banguntapan, Bantul, Daerah Istimewa Yogyakarta 55191, Indonesia

Search Scope

All

Search

Browse

- » [By Issue](#)
- » [By Author](#)
- » [By Title](#)
- » [Other Journals](#)

KEYWORDS

[Backpropagation CNN COVID-19](#)
[Control Distributed Generation](#)
[GLCM Image Processing](#)
[IoT Matlab Monitoring PID](#)
[PLC Prediction RMSE Security](#)
[Sentiment Analysis Sliding](#)
[mode control Technology](#)
[Temperature Thresholding](#)
[Wind Turbine](#)

VISITOR

[View JITEKI stat](#)
0000278541

VISITOR COUNTRY

Visitors

	28,092		282
	2,693		258
	943		198
	429		197
	392		191
	370		147
	337		139
	307		131
	296		128
	289		128

FLAG counter



JURNAL ILMIAH TEKNIK ELEKTRO KOMPUTER DAN INFORMATIKA (JITEKI)

UNIVERSITAS AHMAD DAHLAN

P-ISSN : 23383062 <> E-ISSN : 23383062 Subject Area : Science, Engineering



1.65672
Impact Factor



505
Google Citations



S2
Current
Accreditation

Google Scholar Garuda Website Editor URL

History Accreditation

2016 2017 2018 2019 2020 2021 2022 2023 2024

Garuda Google Scholar

Modification of Control Oil Feeding with PLC Using Simulation Visual Basic and Neural Network Analysis

Universitas Ahmad Dahlan Jurnal Ilmiah Teknik Elektro Komputer dan Informatika Vol 8, No 1 (2022): March 38-50

2022 DOI: 10.26555/jiteki.v8i1.22336 S2 Journal

Multi-hop ESP-Mesh Network and MQTT Protocol for Smart Light Systems in High-Rise Buildings

Universitas Ahmad Dahlan Jurnal Ilmiah Teknik Elektro Komputer dan Informatika Vol 8, No 1 (2022): March 51-63

2022 DOI: 10.26555/jiteki.v8i1.22535 S2 Journal

Detection of Oxygen Levels (SpO2) and Heart Rate Using a Pulse Oximeter for Classification of Hypoxemia Based on Fuzzy Logic

Universitas Ahmad Dahlan Jurnal Ilmiah Teknik Elektro Komputer dan Informatika Vol 8, No 1 (2022): March 17-26

2022 DOI: 10.26555/jiteki.v8i1.22139 S2 Journal

Simulation of Logic Circuit Tests on Android-Based Mobile Devices

Universitas Ahmad Dahlan Jurnal Ilmiah Teknik Elektro Komputer dan Informatika Vol 8, No 1 (2022): March 27-37

2022 DOI: 10.26555/jiteki.v8i1.22200 S2 Journal

Valuation of 5G mmWave Fixed Wireless Access in Residence Area : Analysis of Real Option for Wireless Broadband Service in Kota Wisata Cibubur Using Decision Tree and Black Scholes Model

Modeling and Analysis of Percentage Depth Dose (PDD) and Dose Profile of X-Ray Beam Produced by Linac Device with Voltage Variation

Bilalodin, Farzand Abdullatif

Department of Physics, Faculty of Mathematics and Natural Sciences, Jenderal Soedirman University, Purwokerto 53122, Indonesia

ARTICLE INFO

Article history:

Received March 20, 2022
Revised April 27, 2022
Accepted May 25, 2022

Keywords:

Modelling;
PDD;
Dose profile;
PHITS

ABSTRACT

The Percentage Depth Dose (PDD) and dose profile of X-Ray output from a LINAC therapy device has been modeled and analyzed. The research was conducted by simulation method through the use of the Particle and Heavy Ion Transport System (PHITS) program. The LINAC therapy device modeled in this work refers to the Siemens Primus LINAC therapy device, which is operated at 6 MV, 10 MV, and 18 MV voltages. Determination of PDD was carried at a depth of 0-30 cm and dose profile at a depth of 0-20 cm in a water phantom, placed at 100 cm from the source, which is exposed to a radiation field area of $10 \times 10 \text{ cm}^2$. Results from the LINAC therapy device modeling agree with the actual X-ray apparatus and have produced Bremsstrahlung X-ray. The PDD curve analysis found that the maximum doses are at a depth of 1.5 cm, 2.5 cm, and 3.4 cm. The value of the build-up factor for each LINAC voltage agrees with the reference. Additionally, the results of the analysis of the dose profile suggest that the X-ray output has a good degree of uniformity. The flatness of the dose profile occurs at the depth of 20 cm with a percentage value of flatness at 1.6%, 1.9%, and 1.2%. The flatness values are all less than 2%. The flatness values show a $\leq 2\%$ deviation from the reference value, which is below the tolerance range required in a measurement.

This work is licensed under a [Creative Commons Attribution-Share Alike 4.0](https://creativecommons.org/licenses/by-sa/4.0/)



Corresponding Author:

Bilalodin, Jenderal Soedirman University, Jl. dr. Soeparno Utara 61 Grendeng, Purwokerto 53122, Indonesia
Email: bilalodin@unsoed.ac.id

1. INTRODUCTION

Medical Linear Accelerator (LINAC) is an alternative therapy for cancer or tumors other than Cobalt 60 radiotherapy [1]. The main goal of LINAC radiotherapy is to provide a maximum dose to the tumor and a low dose to healthy cells near the tumor to improve quality of life and prolong patient survival [2]. In order to achieve this goal, the dose distribution produced by LINAC needs to be verified with an accurate method [3]. Two quantities that need to be verified before using the LINAC therapy device are the Percentage Depth Dose (PDD) and the dose profile [4][5].

Verification using a simulation approach is essential before LINAC therapy equipment is set up or prepared for the treatment of the patient [6]. One of the simulation methods to achieve this goal is the Monte Carlo method. The Monte Carlo method has been of great help in planning therapy using various radiation sources [7]. The method can also calculate in detail the spectral energy distribution of particles generated from the LINAC therapy apparatus as well as dosimetric calculations in the form of Percentage Depth Dose (PDD) and dose profiles [8].

Various Monte Carlo-based programs (codes) have been developed, such as MCNP, Geant4, and Penelope. MCNP is a Monte Carlo code developed by the Los Alamos National Laboratory. Geant4 was developed by CERN and KEK laboratories in 1993, and Francesc Salvat and colleagues developed Penelope at the University of Barcelona. In practice, the results vary due to differences in computational systems and in

nuclear data libraries included with the respective MC packages [9]. The weakness of the MCNP program is that it cannot visually display particle traces directly. On the other hand, Geant4 and Penelope are used only in the limited range of energy between 50 eV to 1 GeV [10].

The latest development is a code developed in Japan under Particle Heavy Ion Transport System (PHITS). The PHITS is a Monte Carlo method developed by the Japan Atomic Energy Agency (JAEA) to simulate nuclear processes in various research fields such as dosimetry, accelerator, shield design, space research, medical applications, and material research [11]. The advantage of the PHITS as a Monte Carlo-based program is that it is equipped with a tally that can visualize particle traces in 2 and 3 dimensions and calculate the physical quantity to be determined. The PHITS program is also suitable for simulating the transport of charged and uncharged particles that move randomly within the range of energy from 10^{-4} eV to 1 TeV [12].

The use of the PHITS program in this study contributes to a visual explanation of the mechanism of X-ray generation from the LINAC device and a more accurate determination of the PDD curve and dose profile. The accuracy in determining these parameters is a prerequisite before the LINAC device is used as a therapy instrument.

2. METHOD

The method used in this research is simulation. The research was conducted through several stages. The initial stage is literature and theoretical studies on the LINAC device, particularly the components that make up the LINAC head and important predetermined parameters before therapeutic operation. The following stage models the LINAC device by compiling the PHITS program input. The last stage is simulation to test the validity of the model and the determination of PDD parameters and dose profiles. The stages of the research are shown in Fig. 1.



Fig. 1. Flowchart of modeling and analysis of PDD and dose profile in the research

2.1. Modeling of LINAC Therapy Device

The modeling of the LINAC therapy device is focused on the LINAC head. This section is chosen because it is the place where X-ray is generated. The material composition used in modeling the LINAC head geometry is based on the Siemens Primus LINAC device. Only the main components of the LINAC head are modeled, namely the target, primary collimator, flattening filter, and secondary collimator [13]. The radiation field area used in this study is $10 \times 10 \text{ cm}^2$ and the distance from Source to Skin Distance (SSD) is 100 cm [14]. The components that make up the LINAC head is shown in Table 1.

Table 1. Composition of the material components of the LINAC head [15]

LINAC Head Components	Materials	Percentage (%)	Density (g/cm^3)
Target	Tungsten (184W)	100	19.4
	Tungsten (184W)	90.5	
Primary Collimator	Nickel (58Ni)	6.5	17
	Iron (56Fe)	3	
Flattening Filter	Copper (63Cu)	69.17	8.92
	Copper (65Cu)	30.83	
Secondary Collimator	Tungsten (184W)	90.5	17
	Nickel (58Ni)	6.5	
	Iron (56Fe)	3	

The success of the X-ray head modeling is judged by the evidence of visualizing the traces of X-ray particles from escaping the target, passing through the components of the LINAC head, and penetrating the water phantom. Other evidence is the presence of an X-ray energy spectrum [16]. The geometry model of the LINAC head is shown in Fig. 2(a). The model of the LINAC head and visualization is shown in Fig. 2(b).

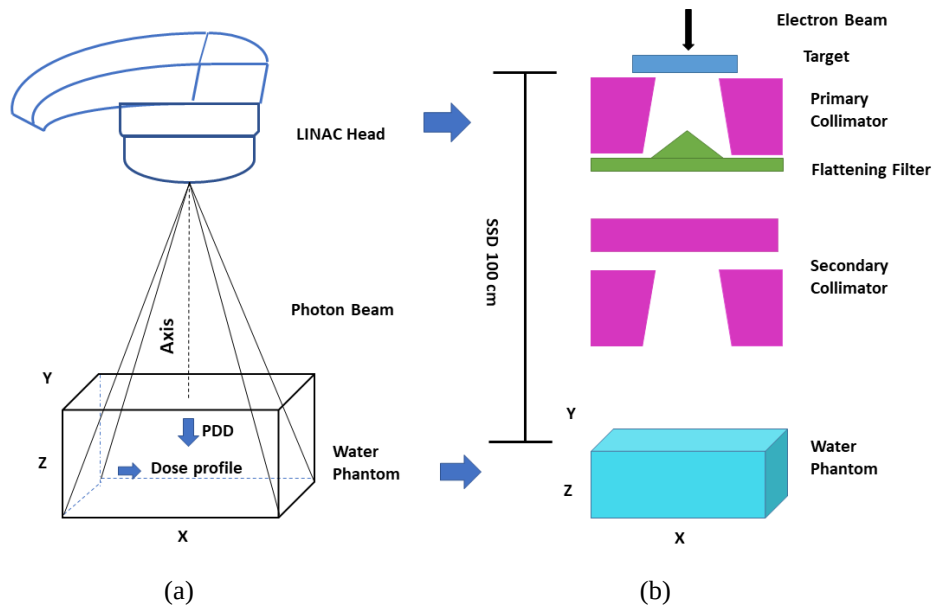


Fig. 2. (a) Geometry of Linac head and water phantom. The x-ray photon beam emitted from the LINAC head is applied to the water phantom. PDD measurement in the direction of the Z-axis and the dose profile perpendicular to the direction of the beam (in the direction of the X-axis), (b) Model of the LINAC head and visualization of the components that make up the LINAC head based on the Simen Primus device

2.2. Determination of PDD Curve and Dose Profile

The standard water phantom determined the PDD curve and the dose profile of the X-ray radiation beam [17]. The water phantom is constructed as a cube of $40 \times 40 \times 40 \text{ cm}^3$ in size. In the phantom, a lattice of voxels (volumetric pixels) are made along the z and x axis. The voxels are designed as small cubes $1 \times 1 \times 1 \text{ cm}^3$ in size. The designed model of the water phantom interposed with voxels is shown in Fig. 3.

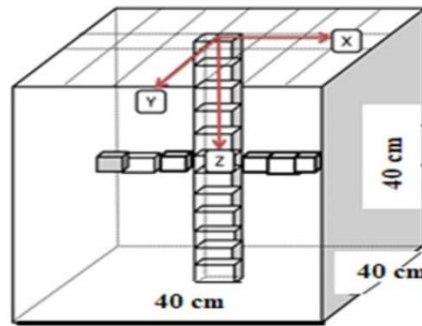


Fig. 3. Geometrical model of water phantom interposed with voxels for measurement of Percentage Depth Dose (PDD) and dose profile

The simulation to determine the PDD curve in the water phantom is carried out at a depth of 0 to 30 cm in the direction of the main axis (z-axis), while the dose profile is determined at a depth that ranges from 0 to 20 cm. The PDD values are calculated at every depth using Eq. (1) [18].

$$PDD = 100 \frac{D_d}{D_{d0}} \quad (1)$$

with D_d is absorption dose at the depth d and D_{d0} is the maximum absorption dose.

Analysis on PDD and dose profile is carried out by finding the difference between the simulation results and the reference value. The stipulated difference is $\leq 2\%$. The flatness value is determined using Eq. (2) [19].

$$Flatness = 100 \frac{D_{max} - D_{min}}{D_{min} + D_{max}} \quad (2)$$

with D_{max} is maximum dose and D_{min} is minimum dose.

The modeling of LINAC head and determination of PDD and dose profile use the PHITS program version 3.24. Visualization of trace particles and X-ray energy spectra uses the *tally tracks*. The determination of PDD values and dose profile, on the other hand, uses the *tally deposit*. The data library for the simulation uses cross sections from the JENDL-4.0 nuclear data library [12].

3. RESULTS AND DISCUSSION

3.1 Modeling The Geometry of LINAC Head

The results of the LINAC head geometry modeling using the PHITS program are shown in Fig. 4. The resulting model needs to be validated to ensure that the model truly represents the actual X-ray equipment. The criteria to ensure the head geometry model represents the actual equipment include the model being able to display the components of the LINAC head, the occurrence of X-rays from the target and their distribution, and the X-ray energy spectrum [16][20].

The high-energy electron beam interaction with the tungsten target produces X-ray radiation with a high-intensity value because tungsten is a target with a high atomic number. Targets with high atoms produce more X-ray radiation than targets with low atomic numbers [21][22].

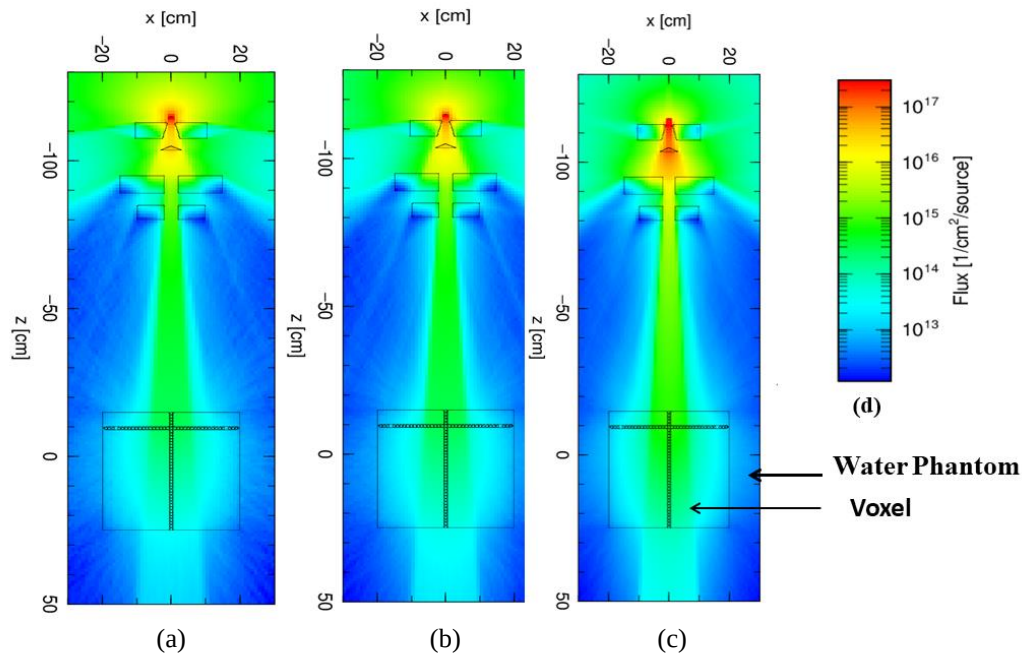


Fig. 4. Traces of X-ray particles produced by LINAC at working voltage of (a) 6 MV (b) 10 MV, and (c) 18 MV. The traces of X-ray particles resulting from the interaction of electrons with the target are depicted in color. Red represents high intensity, and blue represents low intensity, (d) The conversion of intensity in the flux value of X-ray photon

Fig. 3 also shows that the higher the LINAC voltage, the greater the X-ray intensity (shown by, the sharper red color). X-ray Photons generated from the target are passed through the primary collimator, flattening filter, secondary collimator, and water phantom. The X-ray intensity in the area around the target is 10^{16} (p/cm².s) and decreases in intensity when interacting with the primary collimator, flattening filter, and secondary collimator. The X-ray coming out of the secondary collimator decreases in intensity to 10^{15} (p/cm².s) and hit the water phantom with an intensity of 10^{14} (p/cm².s).

The results of the X-ray spectrum from the modeling of the LINAC head are shown in Fig. 5. It can be seen that the X-ray intensity at the three different voltages of the LINAC forms a continuous spectrum. The continuous curve is called the bremsstrahlung curve [23]. The bremsstrahlung curve has maximum peak energy of 0.5 to 1.3 MeV. The maximum energy is generated through the pair production effect and X-rays interacting,

thus creating two annihilating photons, each having an energy of 0.51 MeV [24]. The results are in accordance with those obtained by Baumgartner et al. at the voltage of 10 and 18 MV [25].

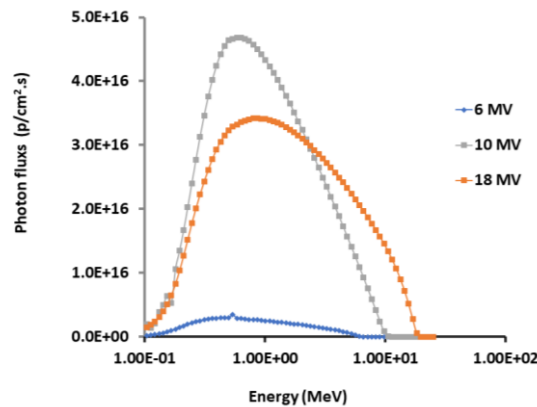


Fig. 5. X-Ray's energy spectrum at various LINAC working voltages. The X-axis represents energy, and the Y-axis represents the number of photon fluxes (X-ray intensity)

3.2 Percentage Depth Dose (PDD) and Dose Profile

3.2.1 Percentage Depth Dose (PDD)

PDD is an important parameter in studying the radiation dose distribution of X-ray photons along the main axis (z-axis) of LINAC. The calculation of PDD is carried out on the surface of the water phantom to a depth of 30 cm. The results of the PDD calculation are shown in Fig. 6, showing that the PDD curve of the three LINAC voltage variations appears to have a uniform graph trend. The PPD curve has a low surface dose pattern, then rises to a maximum value and decreases exponentially. The calculation results of the build-up value at 6, 10, and 18 MV voltages are found at a depth of 1.5 cm, 2.5 cm, and 3.4 cm, respectively.

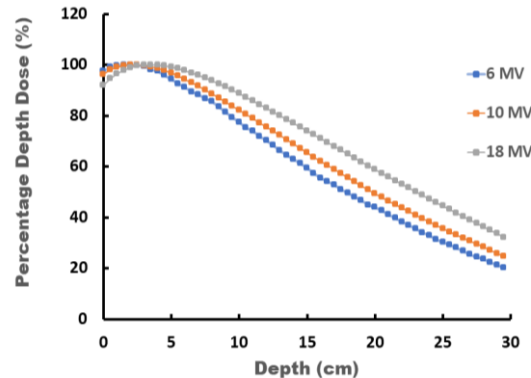


Fig. 6. PDD curve of the three LINAC voltage variations

The build-up value at voltages 6 and 10 MV corresponds to the reference, while 18 MV is smaller than the reference. The difference in the build-up value at 18 MV is 2%. This value is still within the allowable tolerance limit, which is $\leq 2\%$ [26][27]. The maximum dose increases with the LINAC voltage, increasing the X-ray energy produced. X-ray photons can penetrate the water phantom deeper, so the build-up position is increasing [28][29].

3.2.2 Dose Profile

Dose profile refers to the relative dose distribution along the horizontal axis (x-axis) that is perpendicular to the direction of the incident X-ray radiation beam. The profile curve of radiation dose for each variation of LINAC voltage using a radiation field of 10×10 cm and SSD 100 cm is shown in Fig. 6. Fig. 7 shows that the voltage increases the position to reach 100% of the dose gets deeper. The X-rays produced by the LINAC device at voltages of 6, 10, and 18 MV have similar dose profiles. The dose profile tends to decrease as it approaches the edge of the irradiation field. This decrease is due to the penumbra effect [27]. A penumbra

region appears because of X-ray radiation exposure in the radiation field that is limited by the collimator jaws [30][31].

Simulation of dose profile at the voltage of 6, 10, and 18 MV provides different relative doses at 5, 10 and 20 cm depth. At 6 MV, the relative dose at the depth of 5, 10 and 20 cm are respectively 41.5%, 62.2% and 80.1%. At 10 MV, they are 42.2%, 66.7% and 83.4%. At 18 MV, highest values of relative dose are obtained, i.e., 45%, 66.3% and 85.0%. It shows that as the voltage of LINAC increases, the ability of X-ray radiation to penetrate the water phantom correspondingly increases. The increase in penetrating power is due to an increase in the energy of the x-rays [32][33].

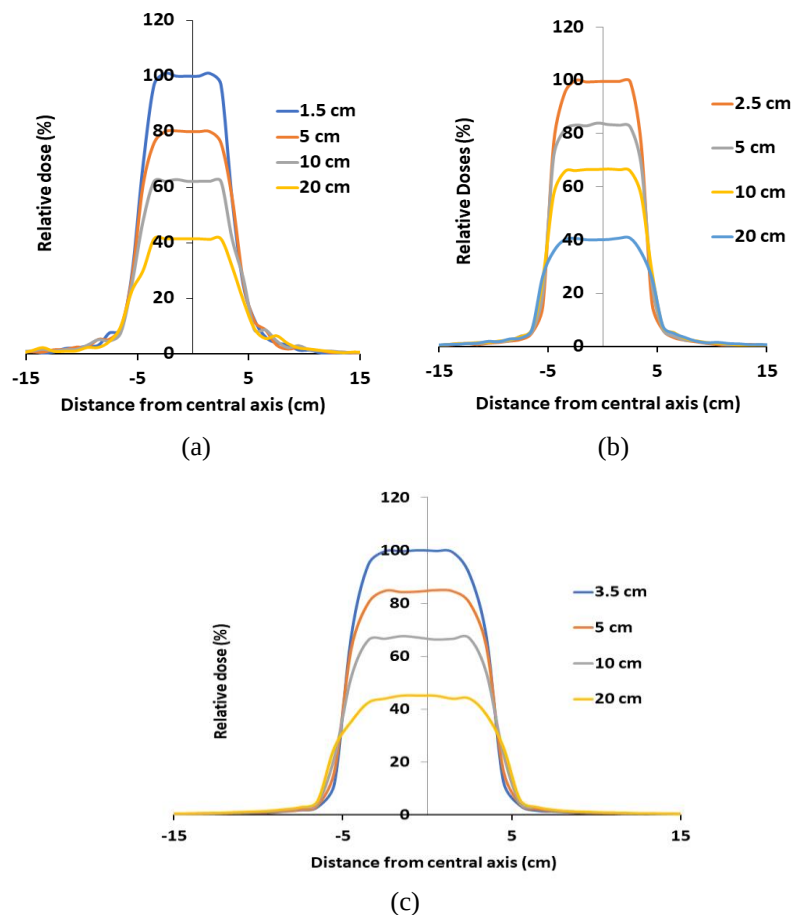


Fig. 7. Dose profile curve produced by LINAC at working voltage of (a) 6 MV (b) 10 MV (c) 18 MV

The degree of uniformity of the photon beam produced by the LINAC machine can be determined from the flatness value of the X-ray beam. The flatness value at the voltage of 6, 10, and 18 MV calculated at a depth of 10 cm is shown in Table 2. The flatness values of the X-ray photon beam are all less than 2%. They are below the permissible flatness value, which is $< 2\%$ [34][35]. However, the dose profile still shows a dose profile that is not symmetrical, as shown in Fig. 6. The area of the left side is not the same as that of the right side. It suggests that the X-ray beams striking the water phantom have different intensities. The difference in intensity is caused by the presence of contaminants in the form of secondary electrons and neutrons that arise when the primary electrons interact with the target [36][37]. The two beams spread out following the X-ray photons. The use of an ion chamber and layered flattening filter is deemed responsible for reducing these contaminants so that the generated X-rays increase the uniformity of the beam [38]–[40].

Table 2. Flatness percentage of a radiation beam

No	Linac (MV)	Percentage of deviation from flatness (%)
1	6	1.6
2	10	1.9
3	18	1.2

4. CONCLUSION

The modeling of the LINAC therapy machine based on the Siemen Primus LINAC device has been successfully carried out. The modeling of the LINAC therapy device agrees with the actual X-ray apparatus. The model of the X-ray therapy device has produced X-ray traces and their spectrum. The calculation of Percentage Depth Dose (PDD) with a radiation field of $10 \times 10 \text{ cm}^2$ at the working voltage of 6, 10, and 18 MV results in maximum doses at a depth of, respectively, 1.5 cm, 2.5 cm, and 3.5 cm. Based on the analysis of the PDD curve, the value of the build-up factor for each LINAC voltage agrees with the reference. The radiation dose profile with a radiation field of $10 \times 10 \text{ cm}^2$ demonstrates that the flatness of the dose profile occurs at the depth of 20 cm with a percentage value of flatness at 1.6%, 1.9%, and 1.2%. The result satisfies the stipulated tolerance limit of $< 2 \%$. For future research, it is necessary to improve the model by adding an ion chamber and a layered flattening filter to the LINAC head component so that the X-ray beam produced is more uniform.

REFERENCES

- [1] B. J. Healy, D. van der Merwe, K. E. Christaki, and A. Meghizifene, "Cobalt-60 Machines and Medical Linear Accelerators: Competing Technologies for External Beam Radiotherapy," *Clin. Oncol.*, vol. 29, no. 2, pp. 110–115, 2017, <https://doi.org/10.1016/j.clon.2016.11.002>
- [2] S. Corradini, F. Alongi, N. Andratschke, C. Belka, L. Boldrini, F. Cellini, and M. Niyazi, "MR-guidance in clinical reality: Current treatment challenges and future perspectives," *Radiat. Oncol.*, vol. 14, no. 1, pp. 1–12, 2019, <https://doi.org/10.1186/s13014-019-1308-y>
- [3] T. Tuğrul and O. Eroğul, "Determination of initial electron parameters by means of Monte Carlo simulations for the Siemens Artiste Linac 6 MV photon beam," *Reports Pract. Oncol. Radiother.*, vol. 24, no. 4, pp. 331–337, 2019, <https://doi.org/10.1016/j.rpor.2019.05.002>.
- [4] T. C. F. Fonseca, B. M. Mendes, M. A. D. S. Lacerda, L. A. C. Silva, L. Paixão, F. M. Bastos, and J. P. R. Junior, "MCMEG: Simulations of both PDD and TPR for 6 MV LINAC photon beam using different MC codes," *Radiat. Phys. Chem.*, vol. 140, pp. 386–391, 2017, <https://doi.org/10.1016/j.radphyschem.2017.03.048>.
- [5] M. R. Bayatiani, F. Fallahi, A. Aliasgharzadeh, M. Ghorbani, B. Khajetash, and F. Seif, "A comparison of symmetry and flatness measurements in small electron fields by different dosimeters in electron beam radiotherapy," *Reports Pract. Oncol. Radiother.*, vol. 26, no. 1, pp. 50–58, 2021, <https://doi.org/10.5603/RPOR.a2021.0009>.
- [6] J. Kim, D. O. Shin, S. H. Choi, S. Min, N. Kwon, U. Jung, and D. W. Kim, "Guideline on Acceptance Test and Commissioning of High-Precision External Radiation Therapy Equipment," *Prog. Med. Phys.*, vol. 29, no. 4, p. 123, 2018, <https://doi.org/10.14316/pmp.2018.29.4.123>.
- [7] B. Faddegon, J. Ramos-Méndez, J. Schuemann, A. McNamara, J. Shin, J. Perl, and H. Paganetti, "The TOPAS tool for particle simulation, a Monte Carlo simulation tool for physics, biology and clinical research," *Phys. Medica*, vol. 72, no. 4, pp. 114–121, 2020, <https://doi.org/10.1016/j.ejmp.2020.03.019>
- [8] T. Gray, N. Bassiri, N. Kirby, S. Stathakis, and K. M. Mayer, "Implementation of a simple clinical linear accelerator beam model in MCNP6 and comparison with measured beam characteristics," *Appl. Radiat. Isot.*, vol. 155, 2020, <https://doi.org/10.1016/j.apradiso.2019.108925>
- [9] J. Fiak, M. Fathi, A. Inchaouh, "Monte Carlo Simulation of a 18 MV Medical Linac Photon Beam Using GATE/GEANT4," *Moscow Univ. Phys.*, vol. 76, pp. 15–21, 2021, <https://doi.org/10.3103/S0027134921010069>
- [10] M. Asai, M. A. Cortés-Giraldo, V. Giménez-Alventosa, V. Giménez Gómez, and F. Salvat, "The PENELOPE Physics Models and Transport Mechanics. Implementation into Geant4," *Front. Phys.*, vol. 9, no. 12, pp. 1–20, 2021, <https://doi.org/10.3389/fphy.2021.738735>.
- [11] T. Furuta and T. Sato, "Medical application of particle and heavy ion transport code system PHITS," *Radiol. Phys. Technol.*, vol. 14, no. 3, pp. 215–225, 2021, <https://doi.org/10.1007/s12194-021-00628-0>.
- [12] T. Sato, Y. Iwamoto, S. Hashimoto, T. Ogawa, T. Furuta, S. I. Abe, and K. Niita, "Features of Particle and Heavy Ion Transport code System (PHITS) version 3.02," *J. Nucl. Sci. Technol.*, vol. 55, no. 6, pp. 684–690, 2018, <https://doi.org/10.1080/00223131.2017.1419890>.
- [13] M. Ghorbani, M. Azizi, B. Azadegan, A. A. Mowlavi, Z. A. Rahvar, and W. Wagner, "Dosimetric evaluation of neutron contamination caused by dental restorations during photon radiotherapy with a 15 MV Siemens Primus linear accelerator," *Radiat. Phys. Chem.*, vol. 174, no. 7, 2019, p. 108961, 2020, <https://doi.org/10.1016/j.radphyschem.2020.108961>.
- [14] R. H. Hasan, S. I. Essa, and M. A. AL-Naqqash, "Depth dose measurement in water phantom for two X-ray energies (6 MeV and 10 MeV) in comparison with actual planning," *Iraqi J. Sci.*, vol. 60, no. 8, pp. 1689–1693, 2019, <https://doi.org/10.24996/ijis.2019.60.8.5>.
- [15] W.M.Abou-TalebaM.H.HassanbE.A.El_MallahcS.M.Kotba, "MCNP5 evaluation of photoneutron production from the Alexandria University 15 MV Elekta Precise medical LINAC," *Appl. Radiat. Isot.*, vol. 135, no. 5, pp. 184–191, 2018, <https://doi.org/10.1016/j.apradiso.2018.01.036>
- [16] M. G. Ahad Ollah Ezzati, Matthew T. Studenski, "Spatial mesh-based surface source model for the electron contamination of an 18 MV photon beams," *J. Med. Phys.*, vol. 45, no. 4, pp. 221–225, 2020, https://doi.org/10.4103/jmp.JMP_29_20.
- [17] W. B. Nurdin, A. Purnomo, and S. Dewang, "Source to Skin Distance (SSD) Characteristics from Varian CX Linear

- Accelerator," *J. Phys. Conf. Ser.*, vol. 979, no. 1, pp. 1–5, 2018, <https://doi.org/10.1088/1742-6596/979/1/012076>.
- [18] G. Martin-Martin, S. Walter, and E. Guibelalde, "Dosimetric impact of failing to apply correction factors to ion recombination in percentage depth dose measurements and the volume-averaging effect in flattening filter-free beams," *Phys. Medica*, vol. 77, no. 8, pp. 176–180, 2020, <https://doi.org/10.1016/j.ejmp.2020.07.006>.
- [19] M. Hossain and J. Rhoades, "On beam quality and flatness of radiotherapy megavoltage photon beams," *Australas. Phys. Eng. Sci. Med.*, vol. 39, no. 1, pp. 135–145, 2016, <https://doi.org/10.1007/s13246-015-0408-8>.
- [20] C. M. Ma, I. J. Chetty, J. Deng, B. Faddegon, S. B. Jiang, J. Li, and E. Traneus, "Beam modeling and beam model commissioning for Monte Carlo dose calculation-based radiation therapy treatment planning: Report of AAPM Task Group 157," *Med. Phys.*, vol. 47, no. 1, pp. 1–18, 2020, <https://doi.org/10.1002/mp.13898>.
- [21] S. Vichi, D. Dean, S. Ricci, F. Zagni, P. Berardi, and D. Mostacci, "Activation study of a 15MeV LINAC via Monte Carlo simulations," *Radiat. Phys. Chem.*, vol. 172, no. 7, p. 108758, 2020, <https://doi.org/10.1016/j.radphyschem.2020.108758>.
- [22] P. Buaphad, Y. Kim, K. Song, H. Dal Park, C. Kim, S. Lee, and J. Ju, "X-ray dose rate estimation model for an electron linac with thick tungsten target," *Nucl. Instruments Methods Phys. Res. Sect. B Beam Interact. with Mater. Atoms*, vol. 498, no. 4, pp. 61–67, 2021, <https://doi.org/10.1016/j.nimb.2021.04.009>.
- [23] T. Almatani, "Validation of a 10 MV photon beam Elekta Synergy linear accelerator using the BEAMnrc MC code," *J. King Saud Univ. - Sci.*, vol. 33, no. 4, p. 101406, 2021, <https://doi.org/10.1016/j.jksus.2021.101406>.
- [24] J. S. E. Jiménez, M. D. Lagos, and S. A. Martinez-Ovalle, "A Monte Carlo Study of the Photon Spectrum due to the Different Materials Used in the Construction of Flattening Filters of LINAC," *Comput. Math. Methods Med.*, 2017, <https://doi.org/10.1155/2017/3621631>.
- [25] A. Baumgartner, A. Steurer, and F. Josef Maringer, "Simulation of photon energy spectra from Varian 2100C and 2300C/D Linacs: Simplified estimates with PENELOPE Monte Carlo models," *Appl. Radiat. Isot.*, vol. 67, no. 11, pp. 2007–2012, 2009, <https://doi.org/10.1016/j.apradiso.2009.07.010>.
- [26] D. E. Krim, D. Bakari, M. Zerfaoui, A. Rrhioa, and Y. Oulhouq, "Monte Carlo evaluation of particle interactions within the patient-dependent part of Elekta 6 MV photon beam applying IAEA phase space data," *Reports Pract. Oncol. Radiother.*, vol. 26, no. 6, pp. 928–938, 2021, <https://doi.org/10.5603/RPOR.a2021.0111>.
- [27] C. Anam, D. S. Soejoko, F. Haryanto, S. Yani, and G. Dougherty, "Electron contamination for 6 MV photon beams from an Elekta linac: Monte Carlo simulation," *J. Phys. Its Appl.*, vol. 2, no. 2, pp. 97–101, 2020, <https://doi.org/10.14710/jpa.v2i2.7771>.
- [28] Y. Li, Y. Gao, X. Liu, J. Shi, J. Xia, J. Yang, and L. Mao, "The influence of beam delivery uncertainty on dose uniformity and penumbra for pencil beam scanning in carbon-ion radiotherapy," *PLoS One*, vol. 16, no. 4, pp. 1–18, 2021, <https://doi.org/10.1371/journal.pone.0249452>.
- [29] A. Das and T. Singha, "Development of a new Monte Carlo based transport code to calculate photon exposure build-up factors in various shielding arrangements," *Radiat. Phys. Chem.*, vol. 194, no. 5, pp. 11–28, 2022, <https://doi.org/10.1016/j.radphyschem.2022.110028>.
- [30] S. Farrukh, N. Ilyas, M. Naveed, A. Haseeb, M. Bilal, and J. Iqbal, "Penumbra Dose Characteristics of Physical and Virtual Wedge Profiles," *Int. J. Med. Physics, Clin. Eng. Radiat. Oncol.*, vol. 6, no. 2, pp. 216–224, 2017, <https://doi.org/10.4236/ijmpcero.2017.62020>.
- [31] N. Qomariyah, R. Wirawan, L. Mardiana, and K. Al Hadi, "Distributions dose analysis for 6 MV photon beams using Monte Carlo-GEANT4 simulation," *AIP Conf. Proc.*, vol. 2169, no. 11, pp. 1–6, 2019, <https://doi.org/10.1063/1.5132656>.
- [32] N. Khaledi, M. Dabaghi, D. Sardari, F. Samiei, F. G. Ahmabad, G. Jahanfarnia, and X. Wang, "Investigation of photoneutron production by Siemens arteis linac: A Monte Carlo Study," *Radiat. Phys. Chem.*, vol. 153, pp. 98–103, 2018, <https://doi.org/10.1016/j.radphyschem.2018.06.006>.
- [33] H. Do Huh and S. Kim, "History of Radiation Therapy Technology," *Prog. Med. Phys.*, vol. 31, no. 3, pp. 124–134, 2020, <https://doi.org/10.14316/pmp.2020.31.3.124>.
- [34] E. Hoseinnezhad, G. Geraily, M. Esfahani, M. Farzin, and S. Gholami, "Comparison of calculated and measured basic dosimetric parameters for total body irradiation with 6- And 18-MV photon beams," *J. Radiother. Pract.*, vol. 20, no. 1, pp. 66–70, 2021, <https://doi.org/10.1017/S1460396919001067>.
- [35] Bn. M. Stimeyra Cana, and Didem Karaçetin, "Beam modeling and commissioning for Monte Carlo photon beam on an Elekta Versa HD LINAC," *Appl. Radiat. Isot.*, vol. 180, no. 1, pp. 11–54, 2022, <https://doi.org/10.1016/j.apradiso.2021.110054>.
- [36] D. Dawn, S. Pal, R. Bakshi, A. K. Kinhikar, R. A. Joshi, K. Jamema, S. V. Datta, "Evaluation of in-field Evaluation of in-field neutron production for medical LINACs with and without flattening filter for various beam parameters - Experiment and Monte Carlo simulation," *Comput. Math. Methods Med.*, vol. 118, no. 11, pp. 98–107, 2018, <https://doi.org/10.1016/j.radmeas.2018.04.005>.
- [37] V. Gracanin, S. Guatelli, D. Cutajar, I. Cornelius, L. T. Tran, D. Bolst, and A. Rosenfeld, "A convenient verification method of the entrance photo-neutron dose for an 18 MV medical linac using silicon p-i-n diodes," *Radiat. Meas.*, vol. 106, no. 2, pp. 391–398, 2017, <https://doi.org/10.1016/j.radmeas.2017.01.004>.
- [38] A. J. Cetnar and D. J. DiCostanzo, "The lifetime of a linac monitor unit ion chamber," *J. Appl. Clin. Med. Phys.*, vol. 22, no. 12, pp. 108–114, 2021, <https://doi.org/10.1002/acm2.13463>.
- [39] A. Zeghari, R. Saaidi, and C. E. M. R., "Linac with Free Flattening Filter Mode," *J Biomed Phys Eng.*, vol. 444, no. 4, pp. 437–444, 2019, <https://doi.org/10.31661/jbpe.v0i0.924>.

- [40] S. Bajwa, A. Gul, S. Ahmed, and M. B. Kakakhel, "Monte Carlo commissioning of radiotherapy LINAC—Introducing an improved methodology," *Reports Pract. Oncol. Radiother.*, vol. 25, no. 5, pp. 720–724, 2020, <https://doi.org/10.1016/j.rpor.2020.06.009>.

BIOGRAPHY OF AUTHORS



Bilalodin received his bachelor degree in Physics from Department of Physics, Universitas Diponegoro, Indonesia, in 1993 and master degree from Physics Department, Institute Teknologi Bandung (ITB), Indonesia, in 2000. Doctoral degree in physics obtained from Universitas Gadjah Mada, in 2000. Current research interest is modeling of therapeutic particles in Medical Physics. Email: bilalodin@unsoed.ac.id



Farzand Abdullatif received his bachelor degree in Physics from Department of Physics, Institut Teknologi Bandung in 1995 and master degree from the same department in 2000. He was awarded doctoral degree from The Australian National University in 2017. His research interest includes Medical Physics and Fluid Dynamics. Email: farzand@unsoed.ac.id



bilalodin 1 <bilalodin@unsoed.ac.id>

Sinta 2 Journal Manuscript Admission Request

2 messages

[JITEKI] <jiteki.maju@uad.ac.id>
Reply-To: "[JITEKI]" <alfianmaarif@ee.uad.ac.id>
To: betaparamita@upi.edu
Cc: betaparamita@upi.edu

Thu, Mar 10, 2022 at 4:06 PM

Dear Friends and Colleagues,

We would like to invite you to submit both original research and review articles to the Jurnal Ilmiah Teknik Elektro Komputer dan Informatika (JITEKI). <http://journal.uad.ac.id/index.php/JITEKI>

The JITEKI welcomes high-quality manuscripts resulting from a research project in the scope of electrical, electronic, computer, informatics, telecommunication, automation, robot, control, power fields.

The manuscript must be original research, written in English, and not be simultaneously submitted to another journal or conference. Submitting Link: <http://journal.uad.ac.id/index.php/JITEKI/login>

The published paper will index in Sinta 2nd Grade, Google Scholar, Crossref Search, Dimensions, Garuda, One Search, PKP Indexed, BASE, WorldCat, Scilit, WorldCat, Index Copernicus International, Research Gate, Moraref. The published paper also has Digital Object Identification (DOI) and a permanent URL.

Important Dates:

Papers Submission Due: 20 March 2022

Review Notification: 30 March 2022

Published Issue: 20 April 2022

You can use the following link for the article journal template

<https://drive.google.com/file/d/16GBDpUapn0ndHq6bsAyqP1LDnpSwksNp/view>

This is a sample of our published article

The Development of Real-Time Mobile Garbage Detection Using Deep Learning

<http://journal.uad.ac.id/index.php/JITEKI/article/view/22295>

Linkage Detection of Features that Cause Stroke using Feyn Qlattice Machine Learning Model

<http://journal.uad.ac.id/index.php/JITEKI/article/view/22237>

We are looking forward to the submission of your paper.

Best Regards,
Assist. Prof. Alfian Ma'arif, M.Eng.
JITEKI Editor
Member of IEEE, ASCEE, PTTI, IAENG
<https://www.scopus.com/authid/detail.uri?authorId=57195619646>
Publication email: alfianmaarif@ee.uad.ac.id

bilalodin 1 <bilalodin@unsoed.ac.id>
To: "[JITEKI]" <alfianmaarif@ee.uad.ac.id>

Sun, Mar 20, 2022 at 11:38 AM

To
The Editor
Jurnal Ilmiah Teknik Elektro Komputer dan Informatika (JITEKI)

.

Dear Sir

I submit the manuscript entitled “Modelling and Analysis of Percentage Depth Dose (PDD) and Dose Profile of X-ray Beam Produced by LINAC Device with Voltage Variation” authored by Bilalodin and Farzand Abdullatif, for the peer-review and publication in your journal “Jurnal Ilmiah Teknik Elektro Komputer dan Informatika”.

The manuscript is our original research work and has been written as well as approved by all authors. It is not submitted to any other journal and under consideration for publication elsewhere, as well as no conflict of interest exists. If it is accepted, it will not be published elsewhere in the same form, in any language, without the written agreement of the publisher.

I have submitted it online. I also attach the manuscript to this email.

Best regards,

Bilalodin
[Quoted text hidden]

 **Manuscript-Bilalodin.docx**
1915K



bilalodin 1 <bilalodin@unsoed.ac.id>

Article revision report

1 message

bilalodin 1 <bilalodin@unsoed.ac.id>
To: "[JITEKI]" <alfianmaarif@ee.uad.ac.id>

Wed, Apr 27, 2022 at 12:57 PM

Dear Editor

I am writing to resubmit our manuscript entitled: **MODELLING AND ANALYSIS OF PERCENTAGE DEPTH DOSE (PDD) AND DOSE PROFILE OF X-RAY BEAM PRODUCED BY LINAC DEVICE WITH VOLTAGE VARIATION** for publication in Jurnal Ilmiah Teknik Elektro Komputer dan Informatika (JITEKI). We would like to thank the editor and reviewer for careful and thorough reading of this manuscript and for the thoughtful comments and constructive suggestions, which help to improve the quality of this manuscript.

The manuscript has been corrected according to Editor and Reviewer suggestion. Repair manuscripts are marked in blue. Revised manuscripts, proof of revision, and Turnitin report are attached. The manuscript has also been gone through grammar check using Grammarly. We hope that this manuscript will be processed until published.

Best regards
Bilalodin

3 attachments

 **Manuscript-Bilalodin proof of article revision.docx**
1019K

 **TURNITIN -manuscript-Bilalodin.pdf**
2434K

 **Manuscript-Bilalodin revised.docx**
1053K



bilalodin 1 <bilalodin@unsoed.ac.id>

[JITEKI] Editor Decision

4 messages

Alfian Ma'arif <alfianmaarif@ee.uad.ac.id>

Thu, Apr 14, 2022 at 9:42 PM

To: Bilal bilalodin - bilalodin <bilalodin@unsoed.ac.id>

Dear bilalodin - bilalodin,

We have reached a decision regarding your submission to Jurnal Ilmiah Teknik Elektro Komputer dan Informatika (JITEKI) with the title, "Modelling and Analysis of Percentage Depth Dose (PDD) and Dose Profile of X-ray Beam Produced by LINAC Device with Voltage Variation"

Our decision is: Revision Required

The detail of the comment is as follow.

Comment of Editor:

>> Please state the research contribution at the end of the introduction, and abstract for example "The research contribution is..." We need at least two research contributions.

The Method contains an explanation of the research method and the proposed method. This section can include research diagrams, system block diagrams, wiring diagrams, or flowcharts diagrams. Please see the guide to make the block diagram or flowchart in the link <https://youtu.be/DN-OdkCMCNM> and <https://youtu.be/spHxAb138xc>

In Results and Discussion section, Please provide a comparison to a similar method from previous works (includes citation) to enhance the research contribution.

The minimal References are 40 from an English Journal that was published 5 years ago and used IEEE Style. The reference must be from IEEE Xplore or Science Direct. All references must have Digital Object Identifier (DOI) or permanent link. See guide to get high quality references from IEEE xplore <https://youtu.be/2dqfF6Xrs8c>

Please use Mendeley to make the references.

The Figure must be in PNG format with 600-1200 dpi. Please don't crop, or use snipping and print-screens tools. Otherwise, the image resolution will be compromised. The images using vector format (EWM) are better.

The Tabel must be made using the Insert Table feature not from the cropping table as an image.

The Equation must be made using Insert Equation. We suggest using 3 columns of the table to help, and then to make the equation in the middle of the column and the number of the equation on the right-side column. The variable in the equation must be given information. Please see the guide in the link on how to make the equation in word and give the equation number. https://youtu.be/O57_TLI5vGA

All of the figures, tables, and equations must be explained, please give some explanation, information, or analysis. All of the figures and tables must be given by

some analysis at least one paragraph.

>> Please use Grammarly to check your manuscript. The free Grammarly is enough for fixing some typos and grammar mistakes. Proofreading is recommended to increase the quality of the English language and writing.

>> Please use the template journal and make sure the percentage of plagiarism is under 25% or the manuscript will be rejected.

>> The minimal pages are 8 included references.

=====

Comment of Reviewers

>>

Please adjust the font, margin, ", / ." with the template and recheck all typo

If there are obstacles and future solutions can be listed or which can be developed from this research

The title must be concise. The abstract must contain 200-300 words that consist of 2-3 sentences about the Introduction, problem, solution; 1-2 sentences about research contribution; 3-4 sentences about the method; 4-5 sentences about the result; and 1-2 sentences about conclusions.

The minimal paragraph in the Introduction is three paragraphs. The introduction section must contain the research problem (at least from 2 journal references), solution, state of the art, novelty, literature review from previous research (at least from 8 references), and research contribution (the most important). Please write the research contribution in the last part of the Introduction such as "The research contribution is...." At least, there are two research contributions.

Commonly, there are research flow, research diagrams, system block diagrams, control system block diagrams, hardware wiring diagrams, pseudocode, or flowcharts in the method section. The figure must be clear, detailed, not blurry, easy to read and provide proper information.

In the results section, provide a comparison to a similar method from previous works (includes citation) to enhance research contributions (compare the result with previous research). All figures and tables must be clear, detailed, not blurry, and easy to read. Each figure and table must be given a comprehensive explanation in at least one paragraph of analysis (crucial).

The conclusions section must be a conclusion, not overview of introduction or results/discussion; written in a paragraph, not in bullets/points. Please add the future work so that it can motivate other researchers to continue the research.

The minimal number of references is 40 and uses the IEEE style. Cited references must be taken from the journal. Each of them should have Digital Object Identifier (DOI) or permanent link. The references were published in the last five years. The references must be from Science Direct, IEEE Xplore, Springer Link, MDPI Scilit, or other reputable databases.

For journal references, please ensure to enlist the name of author (First Name. Last Name), title, journal title, journal volume, article issue number, page number (pp.), published year, and DOI. For example:

[1] A. Ma'arif, A. I. Cahyadi, S. Herdjunto, and O. Wahyunggoro, "Tracking Control of High Order Input Reference Using Integrals State Feedback and Coefficient Diagram Method Tuning," IEEE Access, vol. 8, pp. 182731–182741, Oct. 2020, <https://doi.org/10.1109/ACCESS.2020.3029115>.

Please add the DOI in the references. For example,

E. Widya Suseno and A. Ma'arif, "Tuning of PID Controller Parameters with Genetic Algorithm Method on DC Motor," International Journal of Robotics and Control Systems, vol. 1, no. 1, pp. 41–53, 2021, <https://doi.org/10.31763/ijrcs.v1i1.249>.

=====

Please, login to the JITEKI website and find the PDF / Docx file from a reviewer in the review part.

The author needs to revise the manuscript based on the editor and reviewer's suggestions, advice, and comment. Then, send the revision manuscript using the JITEKI journal website system. Please highlight the change using the yellow/green color in the revised manuscript.

Don't make a new submission, upload it on your previous submission. The maximal file is 2MB.

Thank you,
Best Regards,
Alfian Ma'arif
JITEKI Editor
Universitas Ahmad Dahlan, Indonesia
alfianmaarif@ee.uad.ac.id

bilalodin 1 <bilalodin@unsoed.ac.id>
To: Farzand Abdullatif <farzand@unsoed.ac.id>

Wed, Apr 20, 2022 at 9:35 PM

[Quoted text hidden]

Farzand Abdullatif <farzand@unsoed.ac.id>
To: bilalodin 1 <bilalodin@unsoed.ac.id>

Wed, Apr 20, 2022 at 10:15 PM

Ini yang bahasa Inggrisnya sudah diperbaiki lagi Pak

[Quoted text hidden]

 **Artikel Ilmiah_Ibilalodin PDD-profil dosis - Eng.edited.docx**
1267K

bilalodin 1 <bilalodin@unsoed.ac.id>
To: Farzand Abdullatif <farzand@unsoed.ac.id>

Thu, Apr 21, 2022 at 1:21 PM

Mks Pak , sy perbaiki tabel dan Gambar

[Quoted text hidden]



bilalodin 1 <bilalodin@unsoed.ac.id>

Proof of payment invoice

1 message

bilalodin 1 <bilalodin@unsoed.ac.id>
To: "[JITEKI]" <alfianmaarif@ee.uad.ac.id>

Thu, May 26, 2022 at 7:54 PM

Dear Editor

I am so glad to hear good news.

Thank you very much for accepting my manuscript for publication. We authors express sincere gratitude to Editor and Reviewer for comment and suggestion in order improve my manuscript so that my article can be published.

Proof of payment invoice attached

Best regards

Bilalodin



proof of payment invoice (bilalodin).jpeg
94K